

Instructions for Use

Helicobacter pylori Ag ELISA (stool)

IVD



REF EIA-6120

Σ 96



DRG 

DRG Instruments GmbH, Germany
Frauenbergstraße. 18, 35039 Marburg
Phone: +49 (0)6421-1700 0, Fax: +49 (0)6421-1700 50
Website: www.drg-diagnostics.de
E-mail: drg@drg-diagnostics.de

Distributed by:

DRG 

DRG International, Inc., USA
841 Mountain Ave., Springfield, NJ 07081
Phone: (973) 564-7555, Fax: (973) 564-7556
Website: www.drg-international.com
E-mail: corp@drg-international.com

**Please use only the valid version of the Instructions for Use provided with the kit.
Verwenden Sie nur die jeweils gültige, im Testkit enthaltene, Gebrauchsanweisung.
Si prega di usare la versione valida delle istruzioni per l'uso a disposizione con il kit.
Por favor, se usa solo la version valida de la metodico técnico incluido aqui en el kit.
Utilisez seulement la version valide des Instructions d'utilisation fournies avec le kit.**

Table of Contents

1	INTENDED USE.....	2
2	SUMMARY OF PHYSIOLOGY.....	2
3	ASSAY PRINCIPLE	2
4	REAGENTS: PREPARATION AND STORAGE.....	2
5	SAFETY PRECAUTIONS	3
6	MATERIALS REQUIRED BUT NOT PROVIDED.....	4
7	SPECIMEN COLLECTION & STORAGE.....	4
8	ASSAY PROCEDURE	4
9	PROCEDURAL NOTES	6
10	INTERPRETATION OF RESULTS.....	7
11	LIMITATION OF THE PROCEDURE	7
12	QUALITY CONTROL	7
13	EXPECTED VALUES.....	8
14	EXAMPLE DATA.....	8
15	PERFORMANCE CHARACTERISTICS.....	9
16	REFERENCES / LITERATURE.....	9
17	SHORT ASSAY PROCEDURES.....	10
	SYMBOLS USED.....	11

1 INTENDED USE

This microplate-based ELISA (enzyme linked immunosorbent assay) kit is intended for the quantitative and qualitative detection of *Helicobacter pylori* antigen in feces. The assay is a useful tool in the detection of active *H. pylori* infection. This kit is for in vitro diagnostic use only.

2 SUMMARY OF PHYSIOLOGY

H. pylori (previously known as *Campylobacter pyloridis*) is a type of bacteria that infects the stomach and is a common cause of peptic ulcers. *H. pylori* bacteria can be passed from person to person through direct contact with saliva, vomit or fecal matter. *H. pylori* can also be spread through contaminated food or water.

The infection is normally acquired during childhood. *H. pylori* usually goes undiagnosed until symptoms of a peptic ulcer occur. *H. pylori* infection is quite common and is present in about half the people in the world.

3 ASSAY PRINCIPLE

This “sandwich” ELISA is designed, developed and produced for the quantitative and qualitative measurement of *H. pylori* antigen in stool specimen. The assay utilizes the microplate-based enzyme immunoassay technique by coating highly purified antibody onto the wall of microtiter wells.

Assay calibrators and extracted fecal specimen are added to microtiter wells of microplate that was coated with a highly purified monoclonal *H. pylori* antibody on its wall. During the assay, the *H. pylori* antigen will be bound to the antibody coated plate after an incubation period. The unbound material is washed away and another HRP-conjugated monoclonal antibody which specifically recognizes the protein of *H. pylori* is added for further immunoreactions. After an incubation period, the immunocomplex of “*H. pylori* Antibody – *H. pylori* Antigen – HRP-conjugated Anti-*H. pylori* Tracer Antibody” is formed if *H. pylori* antigen is present in the test sample. The unbound tracer antibody and other proteins in buffer matrix are removed in the subsequent washing step. HRP conjugated tracer antibody bound to the well is then incubated with a substrate solution in a timed reaction and then measured in a spectrophotometric microplate reader. The enzymatic activity of the tracer antibody bound to *H. pylori* proteins captured on the wall of each microtiter well is directly proportional to the amount of *H. pylori* antigen level in each test specimen.

4 REAGENTS: PREPARATION AND STORAGE

This test kit must be stored at 2 °C - 8 °C upon receipt.

For the expiration date of the kit refer to the label on the kit box. All components are stable until this expiration date.

1. *H. pylori* Antibody Coated Microplate

Microplate coated with *H. pylori* antibody.

Qty: 1 x 96 well microplate

Storage: 2 °C - 8 °C

Preparation: Ready to Use.

2. Anti-*H. pylori* Tracer Antibody

HRP-conjugated monoclonal *H. pylori* antibody in a stabilized protein matrix.

Qty: 1 x 12 mL

Storage: 2 °C - 8 °C

Preparation: Ready to Use.

3. ELISA HRP Substrate

Tetramethylbenzidine (TMB) with stabilized hydrogen peroxide.

Qty: 1 x 12 mL

Storage: 2 °C - 8 °C

Preparation: Ready to Use.

4. ELISA Stop Solution

0.5 M sulfuric acid.

Qty: 1 x 12 mL

Storage: 2 °C - 25 °C

Preparation: Ready to Use.

5. H. pylori Antigen Calibrators 1 – 6

Calibrator in bovine serum albumin-based matrix with a proclin preservative.

Qty: 6 x Vials

Storage: 2 °C - 8 °C, <-20°C for long term storage
Do not exceed 3 freeze-thaw cycles.

Preparation: Ready to Use.

H. pylori Antigen Controls

Calibrator in bovine serum albumin-based matrix with a proclin preservative.

Qty: 2 x Vials

Storage: 2 °C - 8 °C, <-20°C for long term storage
Do not exceed 3 freeze-thaw cycles.

Preparation: Ready to Use.

ELISA Wash Concentrate

Surfactant in a phosphate buffered saline with non-azide preservative.

Qty: 1 x 30 mL

Storage: 2 °C - 25 °C

Preparation: 30X Concentrate. The contents must be diluted with 870 mL distilled water and mixed well before use.

6. H. pylori Concentrated Assay Buffer

Concentrated buffer matrix with protein stabilizers and preservative which serves as a patient sample diluent containing a surfactant in phosphate-buffered saline with a non-azide preservative.

Qty: 1 x 30 mL

Storage: 2 °C - 8 °C

Preparation: 4X Concentrate. The contents must be diluted with 90 mL distilled water and mixed well before use.

5 SAFETY PRECAUTIONS

The reagents are for in vitro diagnostic use only.

Source material which contains reagents of bovine serum albumin was derived in the contiguous 48 United States. It was obtained only from healthy donor animals maintained under veterinary supervision and found free of contagious diseases. Wear gloves while performing this assay and handle these reagents as if they were potentially infectious. Avoid contact with reagents containing hydrogen peroxide, or sulfuric acid. Do not get in eyes, on skin, or on clothing. Do not ingest or inhale fumes. On contact, flush with copious amounts of water for at least 15 minutes. Use Good Laboratory Practices.

6 MATERIALS REQUIRED BUT NOT PROVIDED

1. Precision single channel pipettes capable of delivering 10 µL, 25 µL, 50 µL, 65 µL, 100 µL, and 1000 µL.
2. Repeating dispenser suitable for delivering 100 µL.
3. Disposable pipette tips suitable for above volume dispensing.
4. Disposable 12 x 75 mm glass or plastic tubes.
5. Disposable plastic 1000 mL bottle with cap.
6. Aluminum foil.
7. Plastic microtiter well cover or polyethylene film.
8. ELISA multichannel wash bottle or automatic (semi-automatic) washing system.
9. Spectrophotometric microplate reader capable of reading absorbance at 450 nm.

7 SPECIMEN COLLECTION & STORAGE

Fresh fecal sample should be collected into a stool sample collection container.

It is required to collect a minimum of 1-2 mL liquid stool sample or 1-2 g solid sample.

The collected fecal sample must be transported to the lab in a frozen condition (-20 °C). If the stool sample is collected and tested in the same day, it is allowed to be stored at 2 °C - 8 °C.

8 ASSAY PROCEDURE

8.1 Reagent Preparation

1. Prior to use allow all reagents to come to room temperature (20 °C - 25 °C).
Reagents from different kit lot numbers should not be combined or interchanged.
2. Concentrated Assay Buffer must be diluted to working solution prior to use. Please see REAGENTS section for details.
3. ELISA Wash Concentrate must be diluted to working solution prior use. Please see REAGENTS section for details.

8.2 Sample Preparation

8.2.1 For Manual Weighing Procedure Only

1. Patient samples need to be diluted 1:24 with 1x Assay Buffer before being measured.
2. Label a test tube (12 x 75 mm) or a 4 mL plastic vial.
3. With solid stool sample, take or weigh an equivalent amount (about 40 mg, size as a grain of rice) with a spatula or a disposable inoculation loop.
Suspend the solid stool sample with **1 mL 1x Assay Buffer** and mix well on a vortex mixer.
4. Centrifuge the diluted fecal sample at 3000 rpm (800 - 1500 g) for 5 -10 minutes. The supernatant can be directly used in the assay. As an alternative to centrifuging, let the diluted samples sit and sediment for 30 minutes and take the clear supernatant for testing.
5. Note: If the test procedure is performed on an automated ELISA system, the supernatant must be particle-free by centrifuging the sample.
6. This sample can be stored at 2 °C - 8 °C up to three (3) days and below -20 °C for longer storage. Avoid more than 3x freeze and thaw cycle.

8.2.2 Using Fecal Sample Collection Devices, **REF** EIA-6121 or **REF** EIA-6122

1. Label a Fecal Sample Collection tube.
2. Follow the instructions on the Sample Collection Tube insert, **REF** EIA-6121 or **REF** EIA-6122
3. This sample can be stored at 2 °C - 8 °C up to three (3) days and below -20 °C for longer storage. Avoid more than 3x freeze and thaw cycle.
4. Two drops of the extracted sample is equivalent to 100 µL.
5. Note:
H. pylori Sample Collection Test Kit (EIA-6122) is suitable for both automated ELISA system operation and manual assay procedure.
Fecal H. pylori Sample Collection and Extraction Kit (EIA-6121) is most appropriate for manual assay use.

8.3 Quantitative Assay Procedure

1. Place a sufficient number of microwell strips in a holder to run calibrators, controls, and samples in duplicate.
2. Test Configuration

Row	Strip 1	Strip 2	Strip 3
A	Calibrator Level 1	Calibrator Level 5	SAMPLE 1
B	Calibrator Level 1	Calibrator Level 5	SAMPLE 1
C	Calibrator Level 2	Calibrator Level 6	SAMPLE 2
D	Calibrator Level 2	Calibrator Level 6	SAMPLE 2
E	Calibrator Level 3	Control 1	SAMPLE 3
F	Calibrator Level 3	Control 1	SAMPLE 3
G	Calibrator Level 4	Control 2	SAMPLE 4
H	Calibrator Level 4	Control 2	SAMPLE 4

3. Add **100 µL** of calibrators, controls and samples into the designated microwells.
Note: *if the collection tubes from EIA-6121 are used, add two drops of extracted fecal sample into each well.*
4. Cover the plate with one plate sealer and aluminum foil.
Incubate at **room temperature (20 °C - 25 °C)** for **60 minutes**.
5. Remove the plate sealer. Aspirate the contents of each well.
Wash each well **5 times** by dispensing **350 µL** of diluted wash solution into each well, and then completely aspirate the contents. Alternatively, an automated microplate washer can be used.
6. Add **100 µL** of Anti-H.pylori Tracer Antibody to each well. Mix by gently tapping the plate.
7. Cover the plate with one plate sealer and aluminum foil.
Incubate at **room temperature (20 °C - 25 °C)** for **30 minutes**.
8. Remove the plate sealer. Aspirate the contents of each well.
Wash each well **5 times** by dispensing **350 µL** of diluted wash solution into each well, and then completely aspirate the contents. Alternatively, an automated microplate washer can be used.
9. Add **100 µL** of ELISA HRP Substrate into each of the wells. Mix by gently tapping the plate.
10. Cover the plate with one plate sealer and aluminum foil.
Incubate at **room temperature (20 °C - 25 °C)** for **20 minutes**.
11. Remove the aluminum foil and plate sealer.
Add **100 µL** of ELISA Stop Solution into each of the wells. Mix by gently tapping the plate.
12. Read the absorbance at 450/620 nm **within 10 minutes** with a microplate reader.

8.4 Qualitative Assay Procedure

- Place a sufficient number of microwell strips in a holder to run positive control [H.pylori Antigen Calibrator Level 6], negative control [diluted 1X Assay Buffer], and samples in duplicate
- Test Configuration

ROW	Strip 1	Strip 2	Strip 3
A	Negative Control	SAMPLE 3	SAMPLE 7
B	Negative Control	SAMPLE 3	SAMPLE 7
C	Positive Control	SAMPLE 4	SAMPLE 8
D	Positive Control	SAMPLE 4	SAMPLE 8
E	SAMPLE 1	SAMPLE 5	SAMPLE 9
F	SAMPLE 1	SAMPLE 5	SAMPLE 9
G	SAMPLE 2	SAMPLE 6	SAMPLE 10
H	SAMPLE 2	SAMPLE 6	SAMPLE 10

- Add **100 µL** of positive control [H.pylori Antigen Calibrator Level 6], negative control [diluted 1X Assay Buffer], and samples into the designated microwells.
Note: if the collection tubes from EIA-6121 are used, add two drops of extracted fecal sample into each well.
- Cover the plate with one plate sealer and aluminum foil.
Incubate at **room temperature (20 °C - 25 °C)** for **60 minutes**.
- Remove the plate sealer. Aspirate the contents of each well.
Wash each well **5 times** by dispensing **350 µL** of diluted wash solution into each well, then completely aspirate the contents. Alternatively, an automated microplate washer can be used.
- Add **100 µL** Anti-H.pylori Tracer Antibody to each well. Mix by gently tapping the plate.
- Cover the plate with one plate sealer and aluminum foil.
Incubate at **room temperature (20 °C - 25 °C)** for **30 minutes**.
- Remove the plate sealer. Aspirate the contents of each well.
Wash each well **5 times** by dispensing **350 µL** of diluted wash solution into each well, and then completely aspirate the contents. Alternatively, an automated microplate washer can be used.
- Add **100 µL** of ELISA HRP Substrate into each of the wells. Mix by gently tapping the plate.
- Cover the plate with one plate sealer and aluminum foil.
Incubate at **room temperature (20 °C - 25 °C)** for **20 minutes**.
- Remove the aluminum foil and plate sealer.
Add **100 µL** of ELISA Stop Solution into each of the wells. Mix by gently tapping the plate.
- Read the absorbance at 450 nm **within 10 minutes** with a microplate reader.

9 PROCEDURAL NOTES

- It is recommended that all controls and unknown samples be assayed in duplicate. The average absorbance reading of each duplicate should be used for data reduction and the calculation of results.
- Keep light-sensitive reagents in the original amber bottles.
Store any unused antibody coated strips in the foil zipper bag with desiccant to protect from moisture.
Exposure of the plates to humidity drastically reduces the shelf life.
- Careful technique and use of properly calibrated pipetting devices are necessary to ensure reproducibility of the test.
- Incubation times or temperatures other than those stated in this insert may affect the results.
- Avoid air bubbles in the microwell as this could result in lower binding efficiency and higher CV% of duplicate readings.
- All reagents should be mixed gently and thoroughly prior to use. Avoid foaming.

10 INTERPRETATION OF RESULTS

10.1 Quantitative Measurement

1. Calculate the average absorbance for each pair of duplicate test results.
2. Subtract the average absorbance of the Calibrator 1 (0 ng/mL) from the average absorbance of all other readings to obtain corrected absorbance.
3. The calibrator curve is generated by the corrected absorbance of all calibrator levels on the ordinate against the calibrator concentration on the abscissa using a point-to-point or log-log paper. Appropriate computer assisted data reduction programs may also be used for the calculation of results.
4. The *H. pylori* concentrations for the unknown samples are read directly from the calibrator curve using their respective corrected absorbance.

10.2 Qualitative Measurement

Visual:

1. Positive or reactive: Any sample well that is obviously more yellow than the negative control well.
2. Negative or non-reactive: Any sample well that is not obviously more yellow than the negative control well.

Note: The negative control, as well as some patient samples, may show some slight yellow color. A sample well must be obviously darker or more yellow than the negative control well, when it is interpreted as a positive result.

ELISA Reader:

1. Calculate the average absorbance for each pair of duplicate test results.
2. Calculate the cut-off.
Positive Cut-Off = $1.1 \times (\text{mean extinction of negative control} + 0.10)$
Negative Cut-Off = $0.9 \times (\text{mean extinction of negative control} + 0.10)$
3. Interpret test result.
 - Positive: patient sample extinction is greater than the positive Cut-Off.
 - Negative: patient sample extinction is less than the negative Cut-Off.
 - Equivocal: patient sample extinction is between the positive Cut-Off and the negative Cut-Off.
4. Assay quality control.
 - Positive control must show an average OD reading greater than 0.8.
 - Negative control should show an average OD reading less than 0.18.

11 LIMITATION OF THE PROCEDURE

1. The results obtained with this *Helicobacter pylori* Ag (stool) ELISA serve only as an aid to diagnosis and should not be interpreted as diagnostic in themselves without taking other clinical findings such as stomach endoscope and biopsy, etc.
2. Single *H. pylori* negative results in untreated patients do not rule out *H. pylori* infection.
3. For unknown sample value read directly from the assay that is greater than the highest calibrator, it is recommended to measure a further diluted sample for more accurate measurement.
4. Bacterial or fungal contamination of serum specimens or reagents, or cross-contamination between reagents may cause erroneous results.

12 QUALITY CONTROL

To assure the validity of the results each assay should include adequate controls with known *H. pylori* antigen levels. We recommend that all assays include the laboratory's own controls.

13 EXPECTED VALUES

13.1 Quantitative Measurement

Stool from 25 normal adults were measured with this ELISA. We found that normal people show undetectable H. pylori antigen in the extracted stool sample according to the sample collection, extraction and assay procedures described in this insert. The suggested positive cut-off for fecal H. pylori antigen is 3 ng/mL.

13.2 Qualitative Measurement

Stool samples from 29 negative specimens and 17 positive specimens were tested with this ELISA.

Samples DRG's ELISA	True Positive	True Negative	Total
	Positive	0	17
Negative	0	29	29
Total	17	29	46

Sensitivity: 100% (17/17)

Specificity: 100% (29/29)

Accuracy: 100% (46/46)


14 EXAMPLE DATA

14.1 Quantitative Measurement

A typical absorbance data and the resulting calibrator curve from Helicobacter pylori Ag (stool) ELISA are represented.

Note: This curve should not be used in lieu of calibrator curve run with each assay.

Well I.D.	Reading Absorbance (450/620 nm)			Concentration
	Readings	Average	Corrected	
Calibrator Level 1 0 ng/mL	0.047 0.047	0.047	0.000	
Calibrator Level 2 2.1 ng/mL	0.075 0.071	0.073	0.026	
Calibrator Level 3 6.3 ng/mL	0.140 0.144	0.142	0.095	
Calibrator Level 4 18.9 ng/mL	0.357 0.368	0.363	0.316	
Calibrator Level 5 56.7 ng/mL	0.909 0.968	0.939	0.892	
Calibrator Level 6 170 ng/mL	2.682 2.647	2.665	2.618	
Control 1	0.076 0.074	0.076	0.029	2.2
Control 2	0.737 0.711	0.724	0.677	42.6

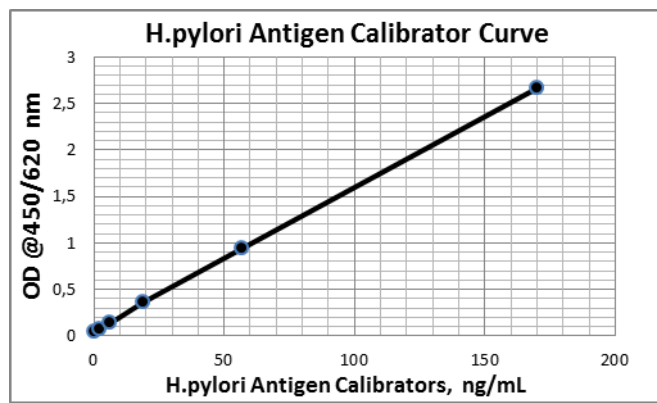

14.2 Qualitative Measurement

	Reading Absorbance (450 nm)	Average
Negative Control	0.049 0.050	0.050
Positive Control	1.332 1.376	1.354

Positive Cut-off = 1.1 × (0.050 + 0.10) = 0.165

Negative Cut-off = 0.9 × (0.050 + 0.10) = 0.135

15 PERFORMANCE CHARACTERISTICS

15.1 Sensitivity

The sensitivity of the Fecal H. pylori Ag ELISA as determined by the 95% confidence limit on 16 duplicate determination of zero standard is approximately 0.165 ng/mL.

15.2 Specificity

The assay does not cross react to the following organisms:
Cryptosporidium parvum, Giardia lamblia, rotavirus and adenovirus.

15.3 Reproducibility and Precision

The intra-assay precision was validated by measuring two samples in a single assay with 12 replicate determinations. The inter-assay precision was validated by measuring two samples in duplicate in 12 individual assays.

Sample	Intra-Assay		Inter-Assay	
	1	2	1	2
Mean (ng/mL)	13.1	1.8	13.9	1.8
CV (%)	5.4	2.8	5.9	5.2

15.4 Linearity

Two (2) stool samples were diluted with assay buffer and tested. The results are as follows:

Samples	Observed (ng/mL)	Recovery (%)
Sample A	77.4	-
50%	38.1	98.4
25%	17.5	90.4
Sample B	24.8	-
50%	12.2	98.6
25%	6.3	102.7

15.5 Spike Recovery

Two samples were spiked with calibrators each other in equal volume and assayed. The results indicate below:

Dilution	Observed (ng/mL)	Recovery (%)
Sample A	0.3	-
+ Level 2: 1.9 ng/mL	1.1	97.2
+ Level 4: 16.7 ng/mL	7.1	84.2
+ Level 5: 50 ng/mL	20.9	83.2
Sample B	0.2	-
+ Level 2: 1.9 ng/mL	1.0	93.8
+ Level 4: 16.7 ng/mL	7.0	82.0
+ Level 5: 50 ng/mL	21.0	83.1

16 REFERENCES / LITERATURE

1. Janoff EN, Smith PD, Blaser MJ. Acute antibody responses to H. Pylori are depressed in patients with AIDS. J Infect Dis. 1988 Apr;157(4):798-804.
2. Rosenblatt JE, Sloan LM, Schneider SK. Evaluation of an enzyme-linked immunosorbent assay for the detection of H. Pylori in stool specimens. Diagn Microbiol Infect Dis. 1993 May-Jun;16(4):337-41.
3. Stibbs HH, Samadpour M, Manning JF. Enzyme immunoassay for detection of H. Pylori cyst antigens in formalin-fixed and unfixed human stool. J Clin Microbiol. 1988 Sep;26(9):1665-9.
4. Stibbs HH. Monoclonal antibody-based enzyme immunoassay for H. Pylori antigen in human stool. J Clin Microbiol. 1989 Nov;27(11):2582-8.
5. Ungar BL, Yolken RH, Nash TE, Quinn TC. Enzyme-linked immunosorbent assay for the detection of H. Pylori in fecal specimens. J Infect Dis. 1984 Jan;149(1):90-7.

17 SHORT ASSAY PROCEDURES

1. Quantitative Measurement

1. Add **100 µL** of the calibrators, controls and samples into the designated microwells.
2. Mix, cover and incubate at **room temperature (20 °C - 25 °C) for 60 minutes.**
3. Wash each well five times.
4. Add **100 µL** of tracer antibody to each well.
5. Cover and incubate at **room temperature (20 °C - 25 °C) for 30 minutes.**
6. Wash each well five times.
7. Add **100 µL** of substrate to each well.
8. Cover and incubate at **room temperature (20 °C - 25 °C) for 20 minutes.**
9. Add **100 µL** of stop solution to each of the wells.
10. Read the absorbance at **450/620 nm**

2. Qualitative Measurement

1. Add 100 µL of positive control [H.pylori Antigen Calibrator Level 6], negative control [diluted 1X Assay Buffer], and samples into the designated microwells.
2. Mix, cover and incubate at **room temperature (20 °C - 25 °C) for 60 minutes.**
3. Wash each well five times.
4. Add **100 µL** of tracer antibody to each well.
5. Cover and incubate at **room temperature (20 °C - 25 °C) for 30 minutes.**
6. Wash each well five times.
7. Add **100 µL** substrate into each well.
8. Cover and incubate at **room temperature (20 °C - 25 °C) for 20 minutes.**
9. Add **100 µL** of stop solution to each of the wells.
10. Read the absorbance at **450 nm.**

SYMBOLS USED

Symbol	English	Deutsch	Italiano	Español	Français
	European Conformity	CE-Konformitäts-kennzeichnung	Conformità europea	Conformidad europea	Conformité normes européennes
	Consult instructions for use *	Gebrauchsanweisung beachten *	Consultare le istruzioni per l'uso	Consulte las instrucciones de uso	Consulter les instructions d'utilisation
	<i>In vitro</i> diagnostic medical device *	<i>In-vitro</i> -Diagnostikum *	Dispositivo medico-diagnostico in vitro	Producto sanitario para diagnóstico In vitro	Dispositif médical de diagnostic in vitro
	Catalogue number *	Artikelnummer *	Numero di Catalogo	Número de catálogo	Référence de catalogue
	Batch code *	Chargencode *	Codice del lotto	Código de lote	Numéro de lot
	Contains sufficient for <n> tests *	Ausreichend für <n> Prüfungen *	Contenuto sufficiente per "n" saggi	Contenido suficiente para <n> ensayos	Contenu suffisant pour "n" tests
	Temperature limit *	Temperaturbegrenzung *	Temperatura di conservazione	Temperatura de conservacion	Température de conservation
	Use-by date *	Verwendbar bis *	Utilizzare prima del	Establa hasta	Utiliser jusque
	Manufacturer *	Hersteller *	Fabbricante	Fabricante	Fabricant
	Caution *	Achtung *			
	For research use only	Nur für Forschungszwecke	Solo a scopo di ricerca	Sólo para uso en investigación	Seulement dans le cadre de recherches
<i>Distributed by</i>	Distributed by	Vertreiber	Distributore	Distribuidor	Distributeur
<i>Content</i>	Content	Inhalt	Contenuto	Contenido	Contenu
<i>Volume/No.</i>	Volume / No.	Volumen/Anzahl	Volume/Quantità	Volumen/Número	Volume/Quantité