

ALL TEST™ HBsAg Rapid Test Dipstick (Serum/Plasma) Package Insert

REF IHBSG-301 English

A rapid test for the qualitative detection of Hepatitis B Surface Antigen (HBsAg) in serum or plasma.

For professional in vitro diagnostic use only.

【INTENDED USE】

The HBsAg Rapid Test Dipstick is a rapid chromatographic immunoassay for the qualitative detection of Hepatitis B Surface Antigen in serum or plasma.

【SUMMARY】

Viral hepatitis is a systemic disease primarily involving the liver. Most cases of acute viral hepatitis are caused by Hepatitis A virus, Hepatitis B virus (HBV) or Hepatitis C virus. The complex antigen found on the surface of HBV is called HBsAg. Previous designations included the Australia or Au antigen¹. The presence of HBsAg in serum or plasma is an indication of an active Hepatitis B infection, either acute or chronic. In a typical Hepatitis B infection, HBsAg will be detected 2 to 4 weeks before the ALT level becomes abnormal and 3 to 5 weeks before symptoms or jaundice develop. HBsAg has four principal subtypes: adw, ayw, adr and ayr. Because of antigenic heterogeneity of the determinant, there are 10 major serotypes of Hepatitis B virus. The HBsAg Rapid Test Dipstick is a rapid test to qualitatively detect the presence of HBsAg in serum or plasma specimen. The test utilizes a combination of monoclonal and polyclonal antibodies to selectively detect elevated levels of HBsAg in serum or plasma.

【PRINCIPLE】

The HBsAg Rapid Test Dipstick is a qualitative, solid phase, two-site sandwich immunoassay for the detection of HBsAg in serum or plasma. The membrane is pre-coated with anti-HBsAg antibodies on the test line region of the Dipstick. During testing, the serum or plasma specimen reacts with the particle coated with anti-HBsAg antibodies. The mixture migrates upward on the membrane chromatographically by capillary action to react with anti-HBsAg antibodies on the membrane and generate a colored line. The presence of this colored line in the test region indicates a positive result, while its absence indicates a negative result. To serve as a procedural control, a colored line will always appear in the control line region indicating that proper volume of specimen has been added and membrane wicking has occurred.

【REAGENTS】

The test Dipstick contains anti-HBsAg particles and anti-HBsAg coated on the membrane.

【PRECAUTIONS】

Please read all the information in this package insert before performing the test.

- For professional in vitro diagnostic use only. Do not use after the expiration date.
- The test should remain in the sealed pouch until ready to use.
- All specimens should be considered potentially hazardous and handled in the same manner as an infectious agent.
- The used test should be discarded according to local regulations.

【STORAGE AND STABILITY】

Store as packaged at room temperature or refrigerated (2-30°C). The test is stable through the expiration date printed on the sealed pouch. The test must remain in the sealed pouch until use. **DO NOT FREEZE.** Do not use beyond the expiration date.

【SPECIMEN COLLECTION AND PREPARATION】

- The HBsAg Rapid Test Dipstick can be performed using serum or plasma.
- Separate serum or plasma from blood as soon as possible to avoid hemolysis. Use only clear non-hemolyzed specimens.
- Testing should be performed immediately after specimen collection. Do not leave the specimens at room temperature for prolonged periods. Serum and plasma specimens may be stored at 2-8°C for up to 3 days. For long term storage, specimens should be kept below -20°C. Collected by venipuncture should be stored at 2-8°C if the test is to be run within 2 days of collection. Do not freeze specimens.
- Bring specimens to room temperature prior to testing. Frozen specimens must be completely thawed and mixed well prior to testing. Specimens should not be frozen and thawed repeatedly.
- If specimens are to be shipped, they should be packed in compliance with federal regulations covering the transportation of etiologic agents.

【MATERIALS】

Materials provided

- Test Dipsticks
- Package insert
- Specimen collection container
- Centrifuge
- Timer

Materials not provided


【DIRECTIONS FOR USE】

- Remove the test dipstick from the sealed foil pouch and use it as soon as possible. Best results will be obtained if the assay is performed immediately after opening the foil pouch.

- For Serum or Plasma specimen: With arrows towards pointing toward serum or plasma specimen, immerse the test Dipstick vertically in the serum or plasma for at least 10-15 seconds. Do not pass the maximum line (MAX) on the test Dipstick when immersing the Dipstick. See illustration below.

- Place the Dipstick on a non-absorbent flat surface, start the timer and wait for the color line (s) to appear. The result should be read at 15 minutes.

Note: A low HBsAg concentration might result in a weak line appearing in the test region (T) after an extended period of time; therefore, do not interpret the result after 30 minutes.

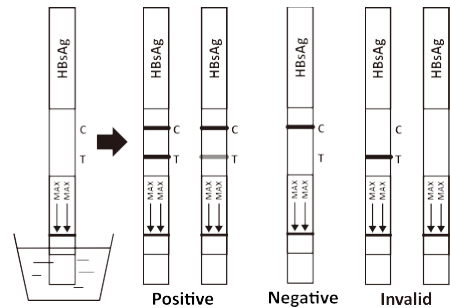

【INTERPRETATION OF RESULTS】

(Please refer to the illustration above)

POSITIVE: Two distinct colored lines appear. One colored line should be in the control region (C) and another colored line should be in the test region (T).

***NOTE:** The intensity of the color in the test line region (T) will vary depending on the concentration of HBsAg present in the specimen. Therefore, any shade of color in the test region (T) should be considered positive.

NEGATIVE: One colored line appears in the control region (C). No apparent colored line appears in the test region (T).

INVALID: Control line fails to appear. Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test Dipstick. If the problem persists, discontinue using the test kit immediately and contact your local distributor.

【QUALITY CONTROL】

A procedural control is included in the test. A colored line appearing in the control region (C) is the internal procedural control. It confirms sufficient specimen volume and correct procedural technique. Control standards are not supplied with this kit; however, it is recommended that a positive control (containing 10ng/ml HBsAg) and a negative control (containing 0ng/ml HBsAg) be tested as a good laboratory practice to confirm the test procedure and to verify proper test performance.

【LIMITATIONS】

- The HBsAg Rapid Test Dipstick is for professional in vitro diagnostic use only. The test should be used for the detection of HBsAg in serum or plasma specimen. Neither the quantitative value nor the rate of HBsAg concentration can be determined by this qualitative test.
- The HBsAg Rapid Test Dipstick will only indicate the presence of HBsAg in the specimen and should not be used as the sole criteria for the diagnosis of Hepatitis B viral infection.
- As with all diagnostic tests, all results must be considered with other clinical information available to the physician.
- The HBsAg Rapid Test Dipstick cannot detect less than 1ng/mL of HBsAg in specimens. If the test result is negative and clinical symptoms persist, additional follow-up testing using other clinical methods is suggested. A negative result at any time does not preclude the possibility of Hepatitis B infection.

【EXPECTED VALUES】

The HBsAg Rapid Test Dipstick (Serum/Plasma) has been compared with a leading commercial HBsAg EIA test. The correlation between these two systems is over 99%.

【PERFORMANCE CHARACTERISTICS】

Sensitivity

The HBsAg Rapid Test Dipstick (Serum/Plasma) has been tested with a sensitivity panel ranging from 0 to 300ng/ml. All 10 HBsAg subtypes produced positive results on The HBsAg Rapid Test Dipstick (Serum/Plasma). The test can detect 1 PEI ng/ml of HBsAg in serum/plasma

Specificity

Antibodies used for the HBsAg Rapid Test Dipstick (Serum/Plasma) were developed against whole Hepatitis B antigen isolated from Hepatitis B virus. Specificity of the HBsAg Rapid Test Dipstick (Serum/Plasma) was also tested with laboratory strains of Hepatitis A and Hepatitis C. They all yielded negative results.

Method	ELISA		Total Results	
	Results	Positive		Negative
	HBsAg Rapid Test Cassette (Serum/Plasma)	Positive		241
	Negative	0	359	359
Total Results		241	361	602

Relative Sensitivity: >99.9% (97.5%CI*: 98.2%-100%)

Relative Specificity: 99.4% (95%CI*: 97.2%-99.8%)

Accuracy: 99.7% (95%CI*: 98.3%-99.9%)

*Confidence Interval

Precision

Intra-Assay

Within-run precision has been determined by using 15 replicates of three specimens containing 0ng/ml, 1ng/ml and 5ng/ml of HBsAg. The negative and positive values were correctly identified 98% of the time.

Inter-Assay

Between-run precision has been determined by using the same three specimens of 0ng/ml, 1ng/ml and 5ng/ml of HBsAg in 15 independent assays. Three different lots of the HBsAg Rapid Test Dipstick (Serum/Plasma) has been tested over a 3-month period using negative, low positive and high positive specimens. The specimens were correctly identified 98% of the time.

Cross-reactivity

The HBsAg Rapid Test Dipstick (Serum/Plasma) has been tested by HAMA, Rheumatoid factor (RF), HAV, Syphilis, HIV, H. Pylori, MONO, CMV, Rubella and TOXO positive specimens. The results showed no cross-reactivity

Interfering Substances

The HBsAg Rapid Test Dipstick (Serum/Plasma) has been tested for possible interference from visibly hemolyzed and lipemic specimens. No interference was observed.

In addition, no interference was observed in specimens containing up to 2,000 mg/dL Hemoglobin, 1000 mg/dL Bilirubin, and 2000 mg/dL human serum Albumin.

【BIBLIOGRAPHY】

- Blumberg, B.S. *The Discovery of Australian Antigen and its relation to viral hepatitis.* *Vitro.* 1971; 7: 22

Index of Symbols

	Attention, see instructions for use		Tests per kit		Do not reuse
	For in vitro diagnostic use only		Use by		Catalog #
	Store between 2-30°C		Lot Number		

Hangzhou AllTest Biotech Co., Ltd.
#550 Yinhai Street
Hangzhou Economic & Technological Development Area
Hangzhou - 310018, P. R. China
www.alltests.com.cn

Number: 145028501
Effective date: 2016-10-08