

ORGENTEC Diagnostika GmbH

Carl-Zeiss-Straße 49-51

55129 Mainz - Germany

Phone: +49 (0) 61 31 / 92 58-0

Fax: +49 (0) 61 31 / 92 58-58

Internet: www.orgentec.com



Electronic Instruction For Use: version



284_2

ORG 284 Lactoferrin

INTENDED PURPOSE

Lactoferrin for Alegria® is an ELISA-based test system for the quantitative measurement of lactoferrin in human stool samples to be used in the assessment of intestinal inflammatory disorders. This product is intended for professional in vitro diagnostic use only.

Elevated faecal lactoferrin levels may be found in patients with chronic inflammatory bowel disease (IBD), and other abdominal disorders, e.g. infectious gastro-enteritis, necrotising enterocolitis, cystic fibrosis, and colorectal carcinoma. Lactoferrin in stool is a sensitive marker for IBD.

SYMBOLS USED

	In vitro diagnostic medical device
	Manufacturer
	Catalogue number
	Sufficient for ... determinations
	Batch code
	Use by
	Temperature limitation
	Consult instructions for use
	Keep away from sunlight
	Do not reuse
	Date of manufacture
	CE marked according to 98/79/EC
	Electronic Instruction For Use: version

	Alegria® Test Strips
	Wash Buffer
	System Fluid
	Ready to use
	Stool Extraction Medium

PRINCIPLE OF THE TEST

Lactoferrin contained in a stool sample has to be released from the stool with stool extraction medium. Then, extracted Lactoferrin can be analyzed with the Alegria® Lactoferrin assay.

The Alegria® assay features barcoded 8-well-microstrips, called Alegria® Test Strips. Each strip is designed for a single determination of one patient sample. The Alegria® Test Strip holds a complete set of reagents. Included are enzyme conjugate, enzyme substrate, sample buffer and a test specific control. Furthermore each strip has two antibody-coated wells which serve as reaction wells for one control and one patient sample.

The determination is based on an indirect enzyme linked immune reaction with the following steps: Lactoferrin present in control / positive samples binds to the surface of the reaction wells forming an antibody-antigen-complex. After incubation, a first washing step removes unbound and unspecifically bound molecules. Subsequently added enzyme conjugate binds to the immobilized antibody-antigen-complex. After incubation, a second washing step removes unbound enzyme conjugate. Addition of enzyme substrate solution results in hydrolysis and colour development during incubation. The intensity of the blue colour correlates with the concentration of the antibody-antigen-complex and can be measured photometrically at 650 nm. The Alegria® Test Strip is based on the proprietary SMC®-Technology (Sensotronic Memorized Calibration): information about the assay, analysis and evaluation, and the lot-specific expiry date is contained on the barcode printed on each Alegria® Test Strip.

The Alegria® Test Strip can be used with the diagnostic instrument Alegria® - a fully automated Random Access Analyser. By means of SMC®-Technology data encoded on the barcode are transferred from the Alegria® Test Strip to the instrument and the assay is automatically processed and evaluated. The instrument reads the date of expiry and rejects further processing if the Alegria® Test Strip is out of date.

WARNINGS AND PRECAUTIONS

- All reagents of this kit are intended for professional in vitro diagnostic use only.
- The control contains material of human origin. Since no test can guarantee the absence of infective agents in human material, we recommend handling Alegria® Test Strips as potentially infective material.
- Bovine serum albumin (BSA) used in components has been tested for BSE and found negative.
- Avoid contact with the substrate TMB (3,3',5,5'-Tetramethyl-benzidine).
- System fluid contains acid, classification is non-hazardous. Avoid contact with skin.
- Control, sample buffer, stool extraction medium and wash buffer contain sodium azide 0.09% as preservative. This concentration is classified as non-hazardous.
- Enzyme conjugate, control and sample buffer contain ProClin 300 0.05% as preservative. This concentration is classified as non-hazardous.

During handling of all reagents, controls and serum samples observe the existing regulations for laboratory safety regulations and good laboratory practice:


- First aid measures: In case of skin contact, immediately wash thoroughly with water and soap. Remove contaminated clothing and shoes and wash before reuse. If system fluid comes into contact with skin, wash thoroughly with water. After contact with the eyes carefully rinse the opened eye with running water for at least 10 minutes. Remove contact lenses if this can be done easily. Get medical attention if necessary. Respiratory tract: take person to the fresh air. Swallowing: Rinse the mouth and spit the fluids out. Drink 1 - 2 glasses of water immediately. During spontaneous vomiting hold the head of the casual low with the body in a prone position in order to avoid the penetration of vomit into the air tube.
- Personal precautions, protective equipment and emergency procedures: Observe laboratory safety regulations. Avoid contact with skin and eyes. Do not swallow. Do not pipette by mouth. Do not eat, drink, smoke or apply makeup in areas where specimens or kit reagents are handled. When spilled, absorb with an inert material and put the spilled material in an appropriate waste disposal.
- Exposure controls / personal protection: Wear protective gloves of nitril rubber or natural latex. Wear protective glasses. Used according to intended use no dangerous reactions known.
- Conditions to avoid: Since substrate solution is light-sensitive. Store Alegria® strips in the dark.
- For disposal of laboratory waste the national or regional legislation has to be observed.

Observe the guidelines for performing quality control in medical laboratories by assaying controls and/or pooled sera.

CONTENTS OF THE KIT

▽ 24 ORG 284

ALEGRIA TEST STRIPS 24



Sufficient for 24 determinations

Alegria® Test Strips are modules of 8 wells each composed of:

Wells 1 + 2: empty and not coated (wells for the sample dilution)

Wells 3 + 4: coated with antibody (reaction wells)

Well 5: **Control**; yellow, containing Lactoferrin, PBS, BSA, detergent, preservative sodium azide 0.09% and ProClin 300 0.05%.

Well 6: **Enzyme Conjugate**; light red, containing anti-Lactoferrin antibodies, HRP labelled; PBS, BSA, detergent, preservative ProClin 300 0.05%.

Well 7: **Sample Buffer**; yellow, containing PBS, BSA, detergent, preservative sodium azide 0.09% and ProClin 300 0.05%.

Well 8: **TMB Substrate**; clear, containing 3,3', 5,5'- Tetramethylbenzidin.

Anti-Lactoferrin antibodies are coated onto microwells.

Code on barcode: **Lactoferrin Stool** on printout: **Lacto**

WASH

1x 20 ml **Wash Buffer**, containing Tris, detergent, preservative sodium azide 0.09%; 50 x concentrate.

SYSTEM FLUID

1x 2.5 ml **System Fluid**, contains acid; 1000 x concentrate.

EXTRACT

1x 20 ml **Stool Extraction Medium**; containing TBS, stabilizing protein, extraction reagent, preservative sodium azide 0.09%. Ready to use. (**F5126**)



1 Certificate of Analysis

MATERIALS REQUIRED

- Vortex mixer, rocking shaker, benchtop centrifuge, optional: precision scales
- Pipettes for 10 µl
- Measuring cylinder for 1000 ml and 2500 ml, microtubes
- Distilled or deionized water

AUXILIARY IVD REAGENTS

- F5126 **EXTRACT** Stool Extraction Medium. This kit component is also available separately.

FURTHER ACCESSORIES

- ORG 282 Stool Extraction Tubes; containing 100 tubes.
- SSCO Stool Sample Collector

These auxiliaries are available separately.

STORAGE AND STABILITY

- Store test kit at 2-8 °C in the dark.
- Do not expose reagents to heat, sun, or strong light during storage and usage.
- Store Alegria® Test Strips sealed and desiccated in the clip bag provided.
- Shelf life of the unopened test kit is 15 months from day of production.
Unopened reagents are stable until expiration of the kit. See labels for individual batch.
- Diluted Wash Buffer and System Fluid are stable for at least 30 days when stored at 2-8 °C.
Once transferred to the reagent container we recommend consumption on the same day.

PROCEDURAL NOTES

- Do not use kit components beyond their expiration dates.
- All materials must be at room temperature (20-28 °C) prior to use.
- To avoid carryover or contamination, change the pipette tip between samples.

SPECIMEN COLLECTION, PREPARATION, STORAGE AND HANDLING

Collecting stool samples

Stool Sample Collector (SSCO) may be used.

- Avoid contamination with toilet water containing disinfectants.
- Keep the collected stool sample no longer than 5 days at 2-8 °C. Alternatively, store at -20 °C.

Preparing stool sample for Extraction

Stool sample and **EXTRACT** have to be at room temperature.

For the Alegria® Lactoferrin assay the stool sample has to be diluted 1:50 in the **EXTRACT** provided.

Inhomogeneous samples should be homogenised prior to sampling, e.g. by using an inoculation loop.

For liquid stool samples we recommend to weigh out sample.

Extraction of Lactoferrin using Stool Extraction Tube (ORG 282)

Prepare Stool **EXTRACT** Tube (ORG 282)

- Fill **750 µl EXTRACT** into the transparent tube to gain a **1:50** dilution.
Use Stool extraction Tubes according to Instruction for Use ORG 282
- Extraction
Vortex 30 sec at 1800 rpm to remove stool sample from the notches of the spatula.
Further homogenize for 15 min at top speed on a rocking shaker.
Open the tube at the blue cone insert and transfer the homogenate to a microtube.
Centrifuge for 2 min at 3000xg. Transfer clear fluid to another microtube and test for Lactoferrin **immediately**.

Extraction of Lactoferrin using other tubes

- Stool sample and **EXTRACT** have to be at room temperature.
- Weigh out empty tube. Pick stool sample and transfer to tube. Weigh out and determine net weight of sample.
- Fill **EXTRACT** into the tube: 49-times net weight of sample needed to gain a 1:50 dilution

stool sample	+	EXTRACT	stool sample	+	EXTRACT
15 mg	+	0.75 ml	60 mg	+	2.9 ml
20 mg	+	1.0 ml	70 mg	+	3.4 ml
30 mg	+	1.5 ml	80 mg	+	3.9 ml
40 mg	+	2.0 ml	90 mg	+	4.4 ml
50 mg	+	2.5 ml	100 mg	+	4.9 ml

Close tube. Vortex 30 sec at 1800 rpm. Further homogenize for 15 min at top speed on a rocking shaker.

Open tube. Transfer the homogenate to a microtube. Centrifuge for 2 min at 3000xg.

Transfer clear fluid to another microtube and test for Lactoferrin **immediately**.

Such an extracted stool sample may be stored at 2-8°C for up to 3 days.

PREPARATION OF REAGENTS

WASH

Dilute the content of the Wash Buffer concentrate (50x) with distilled or deionized water to a final volume of 1000 ml prior to use. Transfer the diluted Wash Buffer into the instrument reagent container.
If only one Alegria run is to be performed on one day we recommend transferring only 500 ml diluted Wash Buffer.

SYSTEM FLUID

Dilute the content of the System Fluid concentrate (1000x) with distilled or deionized water to a final volume of 2500 ml prior to use. Transfer the diluted System Fluid into the instrument reagent container.

ALEGRIA TEST STRIPS

Take the required number of Alegria® Test Strips out of the clip bag and let them reach room temperature (20-28 °C). Do not remove foil covering the empty wells until you are ready to start the assay.

EXTRACT

Ready to use

TEST PROCEDURE

Alegria® Test Strips with SMC® technology are used with the diagnostic instrument Alegria®.

Detailed information about operating the instrument can be taken from the Instrument User Manual.


(1) Remove the foil from the empty wells 1 to 4 of the Alegria® Test Strip.

Do not remove foil with printed barcode, covering wells 5 to 8.

(2) Pipette **100 µl extracted stool sample** at the bottom of well 1.

(3) Insert the strip into the SysTray.

(4) Place loaded SysTrays into the correct position in the Alegria® instrument and start run. All further steps will be done automatically. The test run is completed when the instrument starts printing the results.

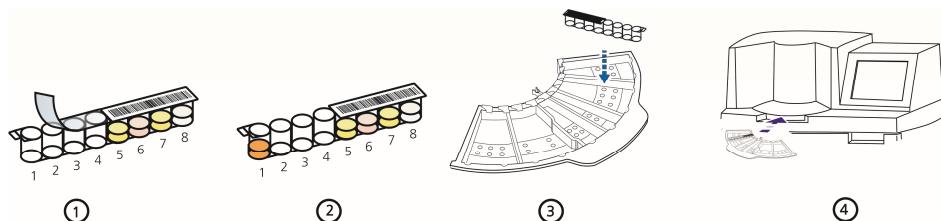

CALIBRATION

The assay system is calibrated using a Lactoferrin reference preparation from human milk.

CALCULATION OF RESULTS

By means of SMC® Technology (Sensotronic Memorized Calibration), all test data are transferred to the system through individual barcodes on the Alegria® Test Strip. Calculation and interpretation of results will be performed automatically.

PERFORMANCE CHARACTERISTICS

Measuring range

The calculation range of this Alegria® assay is 0 - 150 µg/g

Expected values

In a normal range study with samples from healthy donors the following ranges have been established with this Alegria® assay: Cut-off 7.2 µg/g

Interpretation of results

Normal range < 7.2 µg/g
Elevated values > 7.2 µg/g

Lactoferrin level in the normal range: gastrointestinal inflammation nearly ruled out; further invasive diagnostic measures are generally not required.

Lactoferrin level elevated: organic disease of the gastrointestinal tract; further intensive diagnostic tests and treatment by a specialised gastroenterologist are urgently advised.

Linearity

Samples containing Lactoferrin were serially diluted in sample buffer to demonstrate the dynamic range of the assay. Activity for each dilution was calculated by means of SMC® Technology.

Sample	Dilution	Observed	Expected	O/E
		[µg/g]	[µg/g]	[%]
1	1:20	122.7	122.7	100
	1:40	60.7	61.4	99
	1:80	30.0	30.7	98
	1:160	14.5	15.3	94
2	1:20	32.6	32.6	100
	1:40	14.6	16.3	90
	1:80	7.4	8.2	90
	1:160	4.0	4.1	97
3	1:20	63.4	63.4	100
	1:40	31.6	31.7	100
	1:80	15.7	15.9	97
	1:160	7.4	7.9	93

Sensitivity

Lowest detectable concentration: 2.5 µg/g

Reproducibility

Intra-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 20 determinations in a single run. Results for precision-within-assay are shown in the table below.

Inter-assay precision: Coefficient of variation (CV) was calculated for each of three samples from the results of 6 determinations in 3 different runs. Results for run-to-run precision are shown in the table below.

Intra-Assay		
Sample	Mean µg/g	CV
1	15.0	5.8
2	23.9	9.1
3	77.3	7.7

Inter-Assay		
Sample	Mean µg/g	CV
1	26.1	5.7
2	31.8	5.8
3	81.7	10.8

Interfering substances

The following substances were tested per 15 mg of stool sample and were found to be non-interfering: Vancomycin hydrochlorid 0.201 mg, Ciprofloxacin 0.15 mg, Pevazid 0.006 mg, Azathioprine 0.021 mg, Prednisone 0.003 mg, Pentasa 0.399 mg, Vitamin A 2.4 UI, Vitamin C 0.015 mg, Vitamin E 0.03 mg, Vitamin D3 0.33 UI, Hemoglobin 1.749 mg. The following microorganisms were tested at 1.1 x 10⁷ CFU per 15 mg of stool sample and were found to be non-interfering: *E. coli*, *Klebsiella pneumoniae*, *Salmonella enterica*, *Shigella flexneri*, *Yersinia enterocolitica*.

Study results

Study population	n	n_pos	%
Inflammatory bowel disease	235	209	88.9
Abdominal disorders	132	4	3.0
Healthy donors	9	0	0.0

		Diagnostic result		
		Pos	Neg	
ORG 284	Pos	209	4	376
	Neg	26	137	
		235	141	
Sensitivity:				88.9%
Specificity:				97.2%
Overall agreement				92.0%

LIMITATIONS OF THE PROCEDURE

This assay is a diagnostic aid. A definite clinical diagnosis should not be based on the results of a single test, but should be made by the physician after all clinical and laboratory findings have been evaluated concerning the entire clinical picture of the patient. Also every decision for therapy should be taken individually.

The above pathological and normal reference ranges in patient stool samples should be regarded as recommendations only. Each laboratory should establish its own ranges according to ISO 15189 or other applicable laboratory guidelines.

Non-steroidal anti-inflammatory drugs (NSAIDs) induce enteropathy in up to 20-65 % of patients receiving these drugs. NSAID can lead to elevated concentrations of fecal Lactoferrin. In these cases reevaluation of fecal Lactoferrin after stopping NSAIDs should be considered.

REFERENCES

1. Lehmann,F.S., Burri,E., and Beglinger,C., The role and utility of faecal markers in inflammatory bowel disease. Therap.Adv.Gastroenterol. 2015. 8: 23-36.
2. Zhou,X.L., Xu,W., Tang,X.X., Luo,L.S., Tu,J.F., Zhang,C.J., Xu,X., Wu,Q.D., and Pan,W.S., Fecal lactoferrin in discriminating inflammatory bowel disease from Irritable bowel syndrome: a diagnostic meta-analysis. BMC Gastroenterol. 2014. 14: 121.
3. Abraham,B.P. and Kane,S., Fecal markers: calprotectin and lactoferrin. Gastroenterol.Clin North Am 2012. 41: 483-495.
4. Caccaro,R., D'Inca,R., Pathak,S., and Sturniolo,G.C., Clinical utility of calprotectin and lactoferrin in patients with inflammatory bowel disease: is there something new from the literature? Expert Rev Clin Immunol 2012. 8: 579-585.
5. Judd,T.A., Day,A.S., Lemberg,D.A., Turner,D., and Leach,S.T., Update of fecal markers of inflammation in inflammatory bowel disease. J Gastroenterol.Hepatol. 2011. 26: 1493-1499.
6. Lewis,J.D., The utility of biomarkers in the diagnosis and therapy of inflammatory bowel disease. Gastroenterology 2011. 140: 1817-1826.
7. Schoepfer,A.M., Trummler,M., Seeholzer,P., Seibold-Schmid,B., and Seibold,F., Discriminating IBD from IBS: comparison of the test performance of fecal markers, blood leukocytes, CRP, and IBD antibodies. Inflamm. Bowel.Dis. 2008. 14: 32-39.
8. Sutherland,A.D., Geary,R.B., and Frizelle,F.A., Review of fecal biomarkers in inflammatory bowel disease. Dis Colon Rectum 2008. 51: 1283-1291.
9. Walker,T.R., Land,M.L., Kartashov,A., Saslowsky,T.M., Lyerly,D.M., Boone,J.H., and Rufo,P.A., Fecal lactoferrin is a sensitive and specific marker of disease activity in children and young adults with inflammatory bowel disease. J Pediatr Gastroenterol.Nutr 2007. 44: 414-422.
10. Tibble,J.A., Sigthorsson,G., Foster,R., Scott,D., Fagerhol,M.K., Roseth,A., and Bjarnason,I., High prevalence of NSAID enteropathy as shown by a simple faecal test. Gut 1999. 45: 362-366.


Notice to the user (European Union):

Any serious incident that has occurred in relation to the device shall be reported to the manufacturer and the competent authority of the EU Member State in which the user and/or the patient is established .


Change Control

Former version: *ORG 284_IFU_EN_QM150278_2015-03-24_1* Reason for revision: *Introduction electronic IFU on homepage*


1



2



3

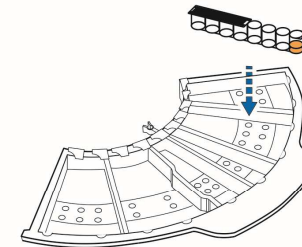

4

